

# PRODUCT CONFORMITY CERTIFICATE

This is to certify that the

## ***OXYMAT 6 Oxygen analyser***

Manufactured by:

### **Siemens AG**

DE-76181  
Karlsruhe,  
Germany

has been assessed by Sira Certification Service  
And for the conditions stated on this certificate complies with:

**MCERTS Performance Standards for Continuous Emission  
Monitoring Systems (CEMS) and T-CEMS, Version 4 dated July 2018  
EN15267-3:2007,  
& QAL 1 as defined in EN 14181: 2014**

Certification Ranges :

O<sub>2</sub>      0 to 5 % vol    to    0 to 25 % vol

Project No.                : 674/0374 & 70211412  
Certificate No            : Sira MC040032/06  
Initial Certification     : 25 February 2004  
This Certificate issued   : 24 February 2019  
Renewal Date            : 24 February 2024

Emily Alexander  
Environmental Project Engineer

MCERTS is operated on behalf of the Environment Agency by

## **Sira Certification Service**

Unit 6, Hawarden Industrial Park  
Hawarden, Deeside, CH5 3US  
Tel: +44 (0)1244 670 900



*The MCERTS certificate consists of this document in its entirety.  
For conditions of use, please consider all the information within.  
This certificate may only be reproduced in its entirety and without change  
To authenticate the validity of this certificate please visit [www.csagroupuk.org/mcerts](http://www.csagroupuk.org/mcerts)*

## Certificate Contents

Approved Site Application.....	2
Basis of Certification .....	2
Product Certified.....	3
Certified Performance .....	4
Description.....	6
General Notes .....	6

## Approved Site Application

*Any potential user should ensure, in consultation with the manufacturer, that the monitoring system is suitable for the intended application. For general guidance on stack emission monitoring techniques refer to Environment Agency Technical Guidance Note M2: Monitoring of stack emissions to air. Operators with installations falling under the Large Combustion Plant Directive or Waste Incineration Directive must refer to Technical Guidance Note M20: Quality Assurance of Continuous Emission Monitoring Systems, for guidance on the suitability of CEMS for their installations. M2 and M20 are available on the Agency's website at [www.mcerts.net](http://www.mcerts.net)*

On the basis of the assessment and the ranges required for compliance with EU Directives this instrument is considered suitable for use on waste incineration and large coal-fired combustion plant applications. This CEM has been proven suitable for its measuring task (parameter and composition of the flue gas) by use of the QAL 1 procedure specified in EN14181, for LCPD and WID applications for the ranges specified. The lowest certified range for each determinand shall not be more than 1.5X the emission limit value (ELV) for WID applications, and not more than 2.5X the ELV for LCPD and other types of application.

The field trial was conducted over 6 months with the Oxymat 6 installed on a waste incinerator.

## Basis of Certification

This certification is based on the following Test Report(s) and on Sira's assessment and ongoing surveillance of the product and the manufacturing process:


TÜV Süddeutschland	Report Number 24019084 dated February 1999
TÜV Süddeutschland	Report Number 13213066 dated April 2009
TÜV Süddeutschland	Report Number 1701476b dated November 2011 (HCl interference)

Certificate No : Sira MC040032/06  
This Certificate issued : 24 February 2019

*This certificate may only be reproduced in its entirety and without change  
To authenticate the validity of this certificate please visit [www.csagroupuk.org/mcerts](http://www.csagroupuk.org/mcerts)*

**Product Certified**

The measuring system consists of the following parts:

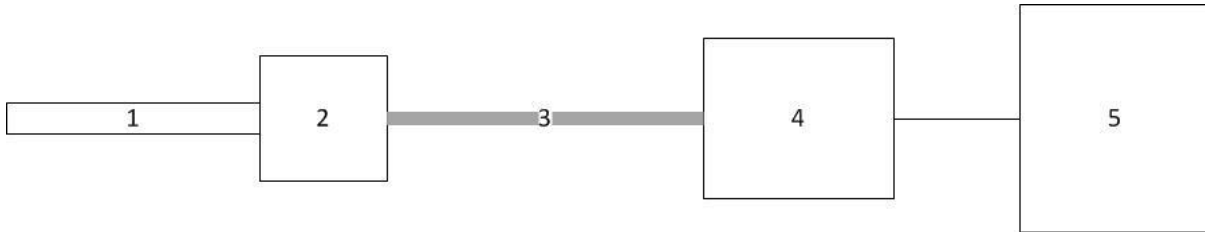

1. Sample Probe	2. Heated Filter	3. Heated Sample Line	4. Gas Conditioning	5. Analyser
Model: M&C SP 2000 HR	Model: Integrated in Sample Probe: S-2K-150	Model: H300 Integral Length: 16m	Model: Sample Cooler M&C/Siemens 7MB1993	Model: OXYMAT 6

Allowable variations could include:

- A different brand or model of sampling system of the same type, provided that there is evidence the alternative system works with similar types of CEM.
- Additional manifolds and heated valves used to allow more than one analyser to share a sampling system.

This certificate applies to all instruments fitted with software version 4 (serial number X2-635) onwards.

Certificate No : Sira MC040032/06  
 This Certificate issued : 24 February 2019

*This certificate may only be reproduced in its entirety and without change  
 To authenticate the validity of this certificate please visit [www.csagroupuk.org/mcerts](http://www.csagroupuk.org/mcerts)*

## Certified Performance

The instrument was evaluated for use under the following conditions:

Ambient Temperature Range: +5°C to +45°C  
 Instrument IP rating: 'E' model IP20  
 'F' model IP40

Note: For outdoor installations the analyser needs to be mounted into an IP65 environment. If the instrument is supplied with an enclosure, then the ambient temperature shall be monitored inside the enclosure to ensure that it stays within the above ambient temperature range.

Unless otherwise stated the evaluation was carried out on the certification range O<sub>2</sub> 0 to 25 % vol

Test	Results expressed as % of the certification range				Other results	MCERTS specification
	<0.5	<1	<2	<5		
Response time					38s	<200s
Repeatability standard deviation at zero point	0.01					<0.2%
Repeatability standard deviation at span point	0.02					<0.2%
Lack-of-fit						
O <sub>2</sub> 0-5 % vol	-0.08					<0.2%
O <sub>2</sub> 0-25 5 vol	-0.05					<0.2%
Influence of ambient temperature zero point – E model	0.12					<0.50%
Influence of ambient temperature zero point – F model	-0.12					<0.50%
Influence of ambient temperature span point - E model	0.14					<0.50%
Influence of ambient temperature span point - F model	0.10					<0.50%
Influence of sample gas flow for extractive CEMS	<0.2					<0.2%
Influence of voltage variations 185 to 264V					No effect	<0.2%
Influence of vibration (10 to 60Hz (±0.3mm), 60 to 150Hz at 19.6m/s <sup>2</sup> )					Not tested	To be reported
Cross-sensitivity at zero	-0.11				Note 1	<0.40%

Certificate No : Sira MC040032/06  
 This Certificate issued : 24 February 2019

*This certificate may only be reproduced in its entirety and without change  
 To authenticate the validity of this certificate please visit [www.csagroupuk.org/mcerts](http://www.csagroupuk.org/mcerts)*

Test	Results expressed as % of the certification range				Other results	MCERTS specification
	<0.5	<1	<2	<5		
Cross-sensitivity at span	0.17				Note 1	<0.40%
Measurement uncertainty (for a range of 25%vol)					0.32%vol	Guidance - at least 25% below max permissible uncertainty
Calibration function (field)					0.99	>0.90
Response time (field)					Note 2 38s	<200s
Lack of fit (field)					Note 3 <0.2%	<0.2%
Maintenance interval					4 weeks	>8 days
Zero and Span drift requirement	<p><u>Statement from manufacturer:</u></p> <p>The zero point is created by purging the measuring cell with an IR-inactive gas (e.g. N<sub>2</sub>) The resulting spectrum corresponds to measurement on a gas free measurement path. The relevant measured concentration values are determined by means of the instrument's calibration function.</p> <p>The span point is created by purging the measuring cell with a gas consisting of the measured component in a concentration of 60-90% of the measuring range, residual gas is IR-inactive N<sub>2</sub> (10-40%). The relevant measured concentration values are determined by means of the instrument's calibration function.</p>					<p>Clause 6.13 &amp; 10.13</p> <p>Manufacturer shall provide a description of the technique to determine and compensate for zero and span drift.</p>
Change in zero point over maintenance interval	0.02					<0.2%
Change in span point over maintenance interval	0.01					<0.2%
Availability					99.3%	>98%
Reproducibility	0.02					<0.20%

Note 1: Cross sensitivity test has been conducted with the following interferents: O<sub>2</sub>, H<sub>2</sub>O, CO, CO<sub>2</sub>, CH<sub>4</sub>, N<sub>2</sub>O, NO, NO<sub>2</sub>, NH<sub>3</sub>, SO<sub>2</sub> and HCl

Note 2: Result stated from laboratory test

Note 3: Test data derived from calibration function test

Certificate No : Sira MC040032/06  
 This Certificate issued : 24 February 2019

*This certificate may only be reproduced in its entirety and without change  
 To authenticate the validity of this certificate please visit [www.csagroupuk.org/mcerts](http://www.csagroupuk.org/mcerts)*

## Description

The OXYMAT 6 gas analysers are based on the paramagnetic alternating pressure sensing method and are used to measure oxygen for 0-5 and 0-25 % vol ranges. This certificate covers three versions of the OXYMAT 6:

- OXYMAT 6E (19 inch rack version)
- OXYMAT 6F (field mounted version)
- OXYMAT 6F (ATEX version) for use in Ex zones 1, 2 and safe areas

The sample chamber is directly in the reference gas stream and has a small volume. Thereby resulting in a short response time.

Corrosion resistance is minimised by the sensor not being exposed to the direct influence of the sample gas. The cell can be cleaned rather than replaced.

Auto calibration is available. Auto or manual range change between four ranges is available. Remote operation of the range change is also possible.

Outputs of 0- 20mA or 4-20mA are standard and a PROFIBUS version can be supplied.

## General Notes

1. This certificate is based upon the equipment tested. The Manufacturer is responsible for ensuring that on-going production complies with the standard(s) and performance criteria defined in this Certificate. The Manufacturer is required to maintain an approved quality management system controlling the manufacture of the certified product. Both the product and the quality management system shall be subject to regular surveillance according to 'Regulations Applicable to the Holders of Sira Certificates'. The design of the product certified is defined in the Sira Design Schedule for certificate No. Sira MC040032/00
2. If certified product is found not to comply, Sira Certification Service should be notified immediately at the address shown on this certificate.
3. The Certification Marks that can be applied to the product or used in publicity material are defined in 'Regulations Applicable to the Holders of Sira Certificates'.
4. This document remains the property of Sira and shall be returned when requested by the company.

Certificate No : Sira MC040032/06  
This Certificate issued : 24 February 2019

*This certificate may only be reproduced in its entirety and without change  
To authenticate the validity of this certificate please visit [www.csagroupuk.org/mcerts](http://www.csagroupuk.org/mcerts)*